


Characteristics

Polymer bonded interior and lightly textured surface, engineered to be slightly thinner for incredible tactile sensitivity and comfort. Unique on-line polymer process creates a glove that's very easy to don without the use of chlorination and very comfortable for extended wear.



**Non-Sterile
Exam Glove**

**ProDerm™
Latex
Series 155**

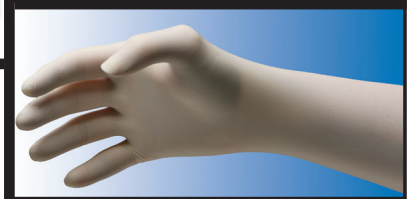

PRODUCT DETAILS

SIZE	ITEM NO.	PACKAGING	DESCRIPTION
XS	155050	100 Gloves/box, 10 boxes/case	Gloves, Exam, Latex, Non Sterile, Powder-Free, Textured
S	155100	100 Gloves/box, 10 boxes/case	
M	155200	100 Gloves/box, 10 boxes/case	
L	155300	100 Gloves/box, 10 boxes/case	
XL	155350	100 Gloves/box, 10 boxes/case	

Product Attributes

- Polymer Dip
- Low Modulus
- Low Protein
- Non-Detectable Residual Chemical Level

Benefits

- Enhanced Donning without Chlorination
- Softer, More Comfortable Fit
- Reduced Chances of Latex Allergic Reactions
- Reduced Chance of Dermatitis and Type IV Reactions

Product Solutions You Trust



ProDerm™

POWDER-FREE | TEXTURED



- *100 Qty (By Weight)*
- *Single Use*
- *Ambidextrous*
- *Non-Sterile*

ProDerm™ is manufactured in compliance with multiple international standards, including the following:

Designation	Standard
ASTM D3578	Standard Specification for Rubber Examination Gloves
ASTM D5151	Standard Test Method for Detection of Holes in Medical Gloves
ASTM F1671	Standard Test Method for Resistance of Materials Used in Protective Clothing to Penetration by Blood-Borne Pathogens
ASTM D5712	Standard Test Method for Analysis of Aqueous Extractable Protein in Natural Rubber

Average Length	Average Palm Thickness	Average Finger Thickness
9.5 in ± 240 mm	4.0 mil ± 0.10 mm	4.5 mil ± 0.11 mm

Tensile Strength & Elongation	Before Aging	After Accelerated Aging
Tensile Strength (Mpa)	28	24
ASTM Requirement Min. (Mpa)	18	14
Elongation (%)	850	820
ASTM Requirement Min. (%)	650	500



Intertek

Innovative Healthcare Corporation is certified to ISO 13485:2003 QMS for medical devices.



4040 Norex Drive, Chaska MN 55318
 phone: 952.448.4412 | fax: 952.448.6180
sales@smithengineeringinc.com
www.smithengineeringinc.com